

(19)



(11)

**EP 1 031 329 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention  
of the grant of the patent:  
**02.07.2008 Bulletin 2008/27**

(51) Int Cl.:  
**A61F 2/06 (2006.01)**

(21) Application number: **00301411.5**

(22) Date of filing: **23.02.2000**

(54) **Bifurcated axially flexible stent**

Abzweigender längsflexibler Stent

Prothèse endovasculaire à flexibilité axiale et avec bifurcation

(84) Designated Contracting States:  
**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU  
MC NL PT SE**

(30) Priority: **24.02.1999 US 256914**

(43) Date of publication of application:  
**30.08.2000 Bulletin 2000/35**

(73) Proprietor: **Cordis Corporation**  
**Miami**  
**FL 33126 (US)**

(72) Inventor: **Hojeibane, Hikmat**  
**Princeton, New Jersey 08540 (US)**

(74) Representative: **Fisher, Adrian John et al**  
**CARPMAELS & RANSFORD**  
**43-45 Bloomsbury Square**  
**London WC1A 2RA (GB)**

(56) References cited:  
**EP-A- 0 904 745 WO-A-00/10485**  
**WO-A-97/41803 WO-A-98/19628**  
**FR-A- 2 733 682 US-A- 5 755 771**  
**US-A- 5 800 508 US-A- 5 893 887**

**EP 1 031 329 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

### Background of the Invention

[0001] A stent is commonly used as a tubular structure left inside the lumen of a duct to relieve an obstruction. Commonly, stents are inserted into the lumen in a non expanded form and are then expanded autonomously (or with the aid of a second device in situ. A typical method of expansion occurs through the use of a catheter mounted angioplasty balloon which is inflated within the stenosed vessel or body passageway in order to shear and disrupt the obstructions associated with the wall components of the vessel and to obtain an enlarged lumen.

[0002] In the absence of a stent, restenosis may occur as a result of elastic recoil of the stenotic lesion. Although a number of stent designs have been reported, these designs have suffered from a number of limitations. These include restrictions on the dimension of the stent such as describes a stent which has rigid ends (8mm) and a flexible median part of 7-21mm. This device is formed of multiple parts and is not continuously flexible along the longitudinal axis. Other stent designs with rigid segments and flexible segments have also been described.

[0003] Other stents are described as longitudinally flexible but consist of a plurality of cylindrical elements connected by flexible members. This design has at least one important disadvantage, for example, according to this design, protruding edges occur when the stent is flexed around a curve raising the possibility of inadvertent retention of the stent on plaque deposited on arterial walls. This may cause the stent to embolize or move out of position and further cause damage to the interior lining of healthy vessels. (See Figure 1(a) below).

[0004] Thus, stents known in the art, which may be expanded by balloon angioplasty, generally compromise axial flexibility to permit expansion and provide overall structural integrity.

[0005] Catheter balloons and medical devices incorporating them are well known for use in the surgical arena. For instance, during angioplasty, stenoses and/or obstructions in blood vessels and other body passageways are altered, in order to increase blood flow through the obstructed area of the blood vessel. For example, in a typical balloon angioplasty procedure, a partially occluded lumen is enlarged through the use of a balloon catheter that is passed percutaneously by way of the arterial system by way to the site of the vascular obstruction. The balloon is then deflated to dilate the vessel lumen at the site of the obstruction.

[0006] Furthermore, another typical procedure uses a "scaffolding," or stent placed on the balloon angioplasty catheter for similar delivery through the arterial system to the site of a vascular obstruction. Thereafter, the balloon angioplasty catheter is inflated, thereby expanding the stent placed on the catheter. When the stent expands, it similarly expands the lumen so that after removal of

the deflated catheter, the stent is retained in its expanded position and thereby holds open that formerly obstructed area of the body passageway.

[0007] Essentially, a balloon catheter is a thin, flexible length of tubing having a small inflatable balloon at a desired location along its length such as at or near its tip. Balloon catheters are designed to be inserted into a body passageway such as the lumen of a blood vessel, a passageway in the heart, a urological passageway, and the like. Typically, the passage of the balloon catheter into the body passageway is done with guidance, such as x-ray or fluoroscopic guidance.

[0008] In practice, stent delivery is quite complex. That is, a stent is sometimes required to be placed in a rather tortuous area of the vasculature. In this instance, it is often necessary to have a catheter which is capable of negotiating tight turns, and/or being placed along a bifurcated length of blood vessel. In some instances, while a generally occluded section of blood vessel can readily be stented, it is often difficult to place a second stent at the other portion of a bifurcation. In other words, one can imagine the bifurcation as an inverted letter "Y" within the body. (The approach of the catheter concerning this inverted "Y" shape is generally through one of the legs in the "Y".) Therefore, the balloon passes both between the leg and the trunk or base of the "Y" rather readily. However, once a stent is placed along these two legs, it is rather difficult to place a second stent at or near the junction of the first leg and the base of the letter "Y". Of course, the same can hold true when the approach is via the base of the "Y" and delivery of the first stent is to one of the legs. This is all the more true because as one advances through the vasculature, the arterial sizes go from quite large (greater than 1cm diameter) to rather small (some time less than 2.5 mm diameter).

[0009] It would be desirable, therefore, to create a system which allows for delivery of a single stent or pair of stents at a bifurcation in the vasculature. It would further be desirable for this stent or for this delivery system to be able to negotiate the bends of the bifurcation, and moreover, to provide for easy access when one stent is already placed. Furthermore, it would be quite useful in order to be able to apply the second stent, for the first stent to be reliably placed every time so that the user knows exactly where the bifurcation is located, and as well where the stent must be appropriately oriented in order to readily access the second leg of the "Y" of the bifurcation.

[0010] Finally, it would be useful for a device such as a desired delivery system to carry a stent capable of allowing secondary access to a bifurcated portion of the vasculature. Thus, it would be most desirable for the device to comprise a catheter capable of balloon delivery of a stent at a bifurcation, and also balloon delivery of a second stent at the bifurcation.

[0011] In FR 2,733,682, there is disclosed a stent of the type set forth in the preamble of the accompanying claim 1.

### summary of the Invention

**[0012]** In accordance with the present invention, there is provided a stent as set forth in the accompanying claim 1.

**[0013]** Further aspects are set out in the dependent claims.

### Brief Description of the Drawings

**[0014]** The foregoing aspects of the invention will be more readily understood by reference to the following detailed description, taken with the accompanying drawings, in which:

**[0015]** Figures 1(a) and 1(b) are side views of a stent having circumferentially disposed bands wherein the stent is in axially unbent and bent positions respectively, the latter showing protruding edges;

**[0016]** Figures 1(c) and 1(d) are side views of an axially flexible stent wherein the stent is in unbent and bent positions respectively, the latter displaying an absence of protruding edges;

**[0017]** Figure 2 is a side view of a portion of the stent of Figures 1(c) and 1(d) showing the longitudinal bands, spaces;

**[0018]** Figures 3 (a) and 3(b) show a portion of the stent of Figure 2 with two bands between two circumferential links (a) before expansion in the unexpanded state; and (b) after expansion, in the deformed state;

**[0019]** Figure 4 is a view along the length of a piece of cylindrical stent (ends not shown) prior to expansion showing the exterior surface of the cylinder of the stent and the characteristic banding pattern;

**[0020]** Figure 5 is an isometric view of a deflection plot where the stent of Figure 2 is expanded to a larger diameter of 5mm;

**[0021]** Figure 6 shows a two-dimensional layout of the stent of Figure 4 to form a cylinder such that edge "A" meets edge "B", and illustrating the spring-like action provided in circumferential and longitudinal directions;

**[0022]** Figure 7 shows a two dimensional layout of the stent. The ends are modified such that the length ( $L_A$ ) is about 20% shorter than length ( $L_B$ ) and the width of the band A is greater than the width of band B;

**[0023]** Figure 8 shows a perspective view of a stent containing flexible connectors;

**[0024]** Figure 9 shows a stent in which the flexible connectors are attached to stent segments, in layout form. These flexible connectors are attached in an every-other-segment pattern;

**[0025]** Figure 10 shows a layout view where the stent segments are connected with a flexible connector in every stent segment pattern;

**[0026]** Figure 11 shows a schematic of the unexpanded stents when loaded on the stent delivery system;

**[0027]** Figure 12 shows the stents placed alone;

**[0028]** Figure 13 shows the stents as expanded without the delivery system;

**[0029]** Figure 14 shows a modification of the stent in a layout view;

**[0030]** Figure 15 is a plan view of the balloon of the present system;

5 **[0031]** Figure 16 is an assembly view of the same balloon;

**[0032]** Figure 17 is a view of the balloon when in use;

10 **[0033]** Figure 18 is a assembly view of a stent in accordance with the present invention which may be used on the balloons of Figures 15-17; and

**[0034]** Figure 19 is a plan view of another stent.

**[0035]** Figures 1(a) to 17, 19 illustrate known stent and balloon configurations, and are included for a clearer understanding of the present invention.

### Detailed Description of Specific Embodiments

**[0036]** Improvements afforded by the disclosed stent configuration illustrated in Figures 1(c) to 10, and not forming a part of the present invention, include (a) increased flexibility in two planes of the non-expanded stent while maintaining radial strength and a high percentage open area after expansion; (b) even pressure on the expanding stent that ensures the consistent and continuous contact of expanded stent against artery wall; (c) avoidance of protruding parts during bending; (d) removal of existing restrictions on maximum of stent; and reduction of any shortening effect during expansion of the stent.

20 **[0037]** Preferably an expandable cylindrical stent 10 may be provided having a fenestrated structure for placement in a blood vessel, duct or lumen to hold the vessel, duct or lumen open, more particularly for protecting a segment of artery from restenosis after angioplasty. The stent 10 may be expanded circumferentially and maintained in an expanded configuration, that is circumferentially rigid. The stent 10 is axially flexible and when flexed at a band, the stent 10 avoids any externally protruding component parts.

40 **[0038]** Figure 1 shows what happens to a stent 10, of a similar design but utilizing instead a series of circumferentially disposed bands, when caused to bend in a manner that is likely encountered within a lumen of the body. A stent 10 with a circumferential arrangement of bands (1) experiences an effect analogous to a series of railroad cars on a track. As the row of railroad cars proceeds around the bend, the corner of each car proceeding around the bend after the coupling is caused to protrude from the contour of the track. Similarly, the serpentine circumferential bands have protrusions (2) above the surface of the stent 10 as the stent 10 bends.

45 **[0039]** The disclosed configuration shown in Figures 1(c) and 1(d) and Figure 7 has bands (3) which are axially flexible and are arranged along the longitudinal axis. This allows the stent to bend so that the bent bands (4) do not protrude from the profile of the curve of the stent 10. Furthermore, any flaring at the ends of the stent 10 that might occur with a stent 10 having a uniform structure is

substantially eliminated by introducing a modification at the ends of the stent 10. This modification comprises decreasing the spatial frequency and increasing the width of the corresponding bands in a circumferential direction ( $L_A$  and  $A$ ) compared to that of the intermediate section. ( $1_B$  and  $B$ ).

**[0040]** The spatial frequency  $L_A$  may be decreased 0-50% with respect to  $L_A$ , and the width  $A$  may be increased in the range of 0-150% with respect to  $B$ . Other modifications at the ends of the stent 10 may include increasing the thickness of the wall of the stent 10 and selective electropolishing. These modifications protect the artery and any plaque from abrasion that may be caused by the stent 10 ends during insertion of the stent 10. The modification also may provide increased radio-opacity at the ends of the stent 10. Hence it may be possible to more accurately locate the stent 10 once it is in place in the body.

**[0041]** The disclosed configuration as shown in Figures 2 and 6 has the unique advantage of possessing effective "springs" in both circumferential and longitudinal directions shown as items (5) and (6) respectively. These springs provide the stent 10 with the flexibility necessary both to navigate vessels in the body with reduced friction and to expand at the selected site in a manner that provides the final necessary expanded dimensions without undue force while retaining structural resilience of the expanded structure.

**[0042]** As shown in both Figures 2, 4 and 6, each longitudinal band undulates through approximately two cycles before there is formed a circumferential link to an adjacent band. Prior to expansion, the wave  $W$  associated with each of the bands may have approximately the same fundamental spatial frequency, and the bands are so disposed that the wave  $W$  associated with them are spatially aligned, so as to be generally in phase with one another as shown in Figure 6.

**[0043]** The aligned bands on the longitudinal axis are connected at a plurality of periodic locations, by a short circumferential link to an adjacent band. Consider a first common axial position such as shown by the line  $X-X$  in Figures 4 and 6. Here an adjacent pair of bands is joined by circumferential link 7. Similarly other pairs of bands are also linked at this common axial position. At a second common axial position, shown in Figure 6 by the line  $Y-Y$ , an adjacent pair of bands is joined by circumferential link 8. However, any given pair of bands that is linked at  $X-X$  is not linked at  $Y-Y$  and vice-versa. The  $X-X$  pattern of linkages repeats at the common axial position  $Z-Z$ . In general, there are thus two groups of common axial positions. In each of the axial positions of any one group are links between the same pairs of adjacent bands, and the groups alternate along the longitudinal axis of the embodiment. In this way, circumferential spring 6 and the longitudinal spring 6 are provided.

**[0044]** A feature of the expansion event is that the pattern of open space in the stent 10 shown in Figure 2 before expansion is different from the pattern of the stent

10 after expansion. In particular, in a preferred embodiment, the pattern of open space on the stent 10 before expansion is serpentine, whereas after expansion, the pattern approaches a diamond shape (3a, 3b). In embodiments of the invention, expansion may be achieved using pressure from an expanding balloon or by other mechanical means.

**[0045]** In the course of expansion, as shown in Figure 3, the wave  $W$  shaped bands tend to become straighter. When the bands become straighter, they become stiffer and thereby withstand relatively high radial forces. Figure 3 shows how radial expansion of the stent 10 causes the fenestrations to open up into a diamond shape with maximum stress being expended on the apices of the diamond along the longitudinal axis. When finite element analyses including strain studies were performed on the stent 10, it was found that maximum strain was experienced on the bands and links and was below the maximum identified as necessary to maintain structural integrity.

**[0046]** The optimization of strain of the stent 10 is achieved by creating as large a turn radius as possible in the wave  $W$  associated with each band in the non-expanded stent 10. This is accomplished while preserving a sufficient number of bands and links to preserve the structural integrity of the stent 10 after expansion. In an embodiment of the invention, the strain may be less than 0.57 for 316L stainless steel. The expansion pressure may be 101.3-709.1 kPa (1.0-7.0 atmospheres). The number of bands and the spatial frequency of the wave  $W$  on the longitudinal axis also affect the number of circumferential links. The circumferential links contribute structural integrity during application of radial force used in expansion of the stent 10 and in the maintenance of the expanded form. While not being limited to a single set of parameters, examples of a stent 10 of the invention having a longitudinal axis and providing axial flexibility of the type shown in Figure 6, may include the following: stents 10 having an expanded diameter of 4mm and a length of 30mm that for example may have about 8-12 rows, more particularly 10 rows; about 6-10 slots, more particularly 8 slots (a slot is shown in Figure 6 as extending between  $X$  and  $Z$ ); and a wave  $W$  amplitude of about  $1/4$ - $1/10$  of a slot length, more particularly  $1/8$  of a slot length.

**[0047]** The stents described may be fabricated from many methods. For example, the stents may be fabricated from a hollow or formed stainless steel tube that may be cut out using lasers, electric discharge milling (EDM), chemical etching or other means. The stents are inserted into the body and placed at the desired site in an unexpanded form. Expansion of the stent may be effected in a blood vessel by means of a balloon catheter, where the final diameter of the stent is a function of the diameter of the balloon catheter used.

**[0048]** The stent can be made at any desired length, most preferably at a nominal 30mm length that can be extended or diminished by increments, for example

1.9mm increments.

**[0049]** It will be appreciated that a stent may be embodied in a shape memory material, including, for example, an appropriate alloy of nickel and titanium; or stainless steel. In such a case after the stent has been formed, it may be compressed so as to occupy a space sufficiently small as to permit its insertion in a blood vessel or other tissue by insertion means, wherein the insertion means include a suitable catheter, or flexible rod. On emerging from the catheter, the stent may be configured to expand into the desired configuration where the expansion is automatic or triggered by a change in pressure, temperature or electrical stimulation.

**[0050]** The stent has utility not only within blood vessels as described above but also in any tubular system of the body such as the bile ducts, the urinary system, the digestive tube, and the tubes of the reproductive system in both men and women.

**[0051]** There is yet further described a stent 10 as presently disclosed containing a multiplicity of curvilinear segments 20. These curvilinear segments 20 are connected to each other via a generally perpendicular connector 25. The generally perpendicular connector 25 lies substantially in the plane perpendicular to the longitudinal axis of the stent 10. Each of the stent 10 segments as described herein is connected to an adjacent stent 10 segment. This is done using a series of flexible connectors. Importantly, the connectors themselves can be made narrower at their midpoints. This enhances the possibility of flexure at that point. Of course, it is to be realized that alternate designs of the connector to insure flexibility are possible, and contemplated by this invention.

**[0052]** In essence therefore, the stent 10 as described in Figure 8 is a stent 10 of considerable flexibility when compared to more rigid rectilinear stents. Nonetheless, the disclosed stent 10 does not depart from the basic concepts set forth herein, in that it discloses a continuously curvilinear strut. This curvilinear strut is connected to other curvilinear struts via a series of "second" more flexible connectors, described above.

**[0053]** In any regard, it can be seen that the disclosed stent 10 incorporates various useful members. One of them is the flexible connector in conjunction with a generally curvilinear stent. Another is the use of the generally larger struts at the ends of the stent 10 in order to provide for continued support at the stent 10 ends. A final aspect is the use of flexible connectors amongst stent 10 segments to provide for greater flexibility.

**[0054]** In all regards, however, it is to be seen that the present invention is to be determined from the attached claims and their equivalents.

**[0055]** As can be seen from Figures 11 through 14, an improved device 100 can also be made to perform in a bifurcated fashion. In this way, the stent 101 contains a central opening 102. This central opening 102 allows for the passage of an unexpanded stent 103 of the same size. Typically of course, the two stents 101, 103 will have the same general configuration, and one can pass

through the other on the same type of diameter balloon. In fact, the balloon 150 as seen in the current figures 11-16 is a bifurcated balloon, but need not be. Two separate balloons are certainly capable of performing the same function. The balloons are preferably less than 2.0 mm (6 Fr) in their unexpanded shape in a preferred embodiment, but of course, need not be so constrained.

**[0056]** As seen in figures 11-14, the first stent 101 (the lower one in the figure) is loaded on one of the balloons 151. It has an opening 102 central to it. This opening faces the upper stent 103 and balloon 152, the upper stent 102 loaded on the second balloon 152. The upper stent 103, when loaded on the second balloon 152 also has an opening 104 which faces the lower stent 101. In this fashion, as the second stent 103 is strung through the first stent 101, it is placed in such a fashion so as to have a mutually facing contact with the first stent 101. Then, as the balloon and stent combination is guided through the human anatomy, the devices will go toward a bifurcation. When this happens, the device is caused to split using various guide wire techniques. Then, each of the respective balloons is inflated.

**[0057]** On this inflation, the entire device is expanded such as seen in Figure 13. Thus, the entire bifurcation is covered, and yet in a much easier than typical bifurcated expansions. What is unique is that there is no welding of the stents 101, 103 together, they can be common "off-the-shelf" stents modified only slightly so as to be useful for this particular need.

**[0058]** It should be noted that the stent of Figures 11-14 can be designed with any slot or wire configurations or of any high density materials or composites and can be balloon expandable or self-expanding or even the combination of both. The devices can be sold separately from separate catheters to be assembled during the desired procedure by the clinicians; can be used with a bifurcated balloon or two separate balloons; or incorporated with one or more radio-opaque markers to allow for better positioning in radio-opacity. The bifurcated stent delivery system is placed by crimping over two balloons and then expanded at the sight of the lesion.

**[0059]** As seen from Figures 15-17, there is described a balloon 510, in which is contained a standard balloon catheter 520. These catheters are described in, for instance, U.S. Patent Nos. 5,108,415; 5,156,612 and 5,304,197, incorporated herein by reference. Uniquely, however, the balloon 510 contains a side hole 515 in the balloon. The side hole 515 is placed at an exit port 516 in the middle 517 of the balloon 510. This side hole 515 creates access to a lumen 525 created in the side of the catheter 510. Thus, this side hole 515 creates an access channel useful for the stent 101 of the current invention.

**[0060]** So in use therefore, the catheter 510 is advanced into the lumen of the artery, as would be typical angioplasty catheter. First, a guidewire 550 is placed within lumen 530 of the catheter 510. Second, the catheter 510 is tracked over the guidewire and into the lumen. Then, the guidewire 550, specially formed for this use is

retracted until its tip 555 is placed at the distal marker 535 of the current catheter 516. Then, the guidewire 550 is rotated so that its tip 555 "pops" out of the side hole 515 created in the side lumen 525 of the present catheter 510. The guidewire 550 is then advanced through the side branch artery to give access to the side branch.

**[0061]** In Figure 18, the first item described will be the structure of stent 200 in accordance with the invention and illustrated in figure 18. The stent 200 is an improvement over other bifurcated stent ideas, in that the stent is continuous through the mid-section 250 of the main branch segment 210, 220. Segment 230 is connected by a spot weld formed between a dowel 261 and a hole 262 to another section 220 to form the "Y"-shaped stent. Such design will allow for greater vessel coverage at the intersection point of the bifurcation.

**[0062]** As was mentioned earlier, stent 200 comprises three tubular sections (210, 220, and 230) and a continuous connection (240). Sections 210, 220, 230 have struts 211, 221, 231 of sinusoidal shape. Of course, any known shape (e.g., straight struts, are possible).

**[0063]** The first section (210) is a proximal section having as its center axis L. It is intended for insertion into main stem of blood vessel for treatment upstream of a bifurcation.

**[0064]** The first distal section (220) having as its section axis L' is at least approximately aligned with proximal section 210 prior to use. This first distal section 220 is intended for insertion to a blood distal branching off from the bifurcation from a proximal blood vessel, into which section 210 is to be placed. The first distal section (220) is attached to proximal section 210 by some of the omega-shaped connector members 250 seen in Figures 18. Omega-shaped connectors 250, it should be realized, are of different shape than struts 211, 221; these omega-shaped connectors 250 are formed to maximize flexibility.

**[0065]** The second distal section (230) having as its axis L" is positioned at the side of the first distal section 220, and has the advantage of being parallel to the latter prior to use. The second distal section 230 is intended to be inserted into a second distal blood vessel branching off from the bifurcation.

**[0066]** The two distal sections 220 and 230 have their proximal ends linked by the connection member 260, which is a weld joint comprising elements 261, 262 seen in Figure 18. Dowel 261 fits into hole 262 to form weld 260.

**[0067]** Each of section 210, 220, and 230 is preferably formed from a tubular component perforated with a slotted tubular pattern such that the structure of sections 210, 220, 230 allows them to expand along their circumferences.

**[0068]** In practice section 210, 220, and 230 of stent is 200 can be manufactured from extruded cylindrical parts made of a bendable metal alloy such as 316L stainless steel, but may also be made from other known metals such as nitinol. The external diameter of sections 210, 220, 230 typically ranges from 1mm to 4mm prior to use,

and =an be expanded further than 2mm and 8mm.

**[0069]** Sections 210, 220 are preferably manufactured from a single tubular part in which flexible connectors, such as omega-shaped connectors 250 are formed via machining.

**[0070]** Weld points 261, 262 are preferably joined by means of, for example, laser welding, or other acceptable alternatives.

**[0071]** Furthermore, proximal end 235 of the second distal section 230 may be tapered at the other side of the connector 250. It extends forward in its peripheral area opposite the omega-shaped connectors 250. This tapered portion may also be determined by a plane that is inclined with reference to L' perpendicular to the plane of symmetry of the stent 200.

**[0072]** After expansion, when the stent 200 is installed at the a bifurcation of the two vessels, distal portion 215 of the proximal section 210 is fit together with the proximal ends 225, 235, of sections 220, 230 of the stent, and ensures maximum coverage of the dilated bifurcation area. This is especially true since weld 260 holds the relative position of sections 220, 230 and the relative positions of sections 210, 220 is set, and covered by omega-shaped connectors 250.

**[0073]** In this way, once in place, the whole of the grid of the bifurcated stent 200 covers the proximal and distal portions of the two branching vessels and the whole of the dilated bifurcation area.

**[0074]** The stents themselves can be made from any high density material or composite. These stents can be balloon expandable or self-expanding or a combination of both. They can be used on catheters as described herein or on standard catheters.

**[0075]** Typical angioplasty catheters contain a central lumen useful for stringing a guidewire therethrough. The guidewire then guides the balloon from a point outside the body, along its length, to a point which is about to be stented. The balloon of the angioplasty catheter holds the stent as it is guided through the vasculature. When the obstruction is reached, the balloon is inflated, the stent is similarly inflated, and then the balloon can be deflated. Upon deflation, the balloon can be retracted through the vasculature along the guidewire.

**[0076]** In a stent delivery system for use with the stent of the present invention, a second guidewire lumen is placed at least within the balloon. (It should also be realized that the second guidewire lumen also can readily be placed along a length of the catheter shaft.) This second guidewire lumen is useful for attacking the bifurcated vessel. What occurs, therefore, is the following: a large stent is placed on the balloon so modified. Thereafter, the guidewire is tracked through the body to a point past the obstruction, which for the purposes described herein, is presumed to occur at or near a bifurcation. Onto the guidewire is tracked the modified stent delivery system. The balloon guidewire lumen is placed on to the guidewire outside the body and it is then moved along the guidewire to a point inside the body. The exit portion

of the second balloon guidewire lumen is somewhere proximal to the distal end of the balloon, so that the entire balloon can be moved to a position along the vasculature at the obstruction in the body passageway.

[0077] When the obstruction is reached, the balloon can be inflated. This will usually take care of the "base" and one of the "legs" of the bifurcation. When inflated, a stent which is associated with the stent delivery system is similarly inflated. This stent has an opening situated along a portion of its wall. This opening is useful for opening the second leg of the bifurcated area.

[0078] The second area is opened in the following manner: a second balloon angioplasty catheter, this time containing a single basic stent is placed along the guidewire during positioning of the balloon catheter. A second guidewire is then strung through the catheter to a position where it emerges from the second opening. Then, the second catheter is guided along the second guidewire so that it, too, is placed along the second guidewire after the guidewire emerges from the distal opening of the balloon second guidewire opening. Then, the second catheter can be inflated when it is resident in the second "leg" of the bifurcation. At that point, because the first leg has already been expanded and the base of the bifurcation has been expanded, once the second leg of the bifurcation is expanded, the entire bifurcation has been attended to and the patient is properly stented.

[0079] Further, there is disclosed a method of stent placement which comprises first guiding a guidewire through the vasculature. Second, a balloon catheter which contains two guidewire lumens is strung along the guidewire into position at the bifurcation. The distal opening of the second guidewire lumen abuts the proximal end of the bifurcation. Thereafter, a second guidewire is strung through the first balloon catheter and out the distal opening of the second guidewire lumen. Thus, resident in the second bifurcation leg is the second guidewire. Then, a second standard stent delivery balloon catheter is guided along the second guidewire to a position within the bifurcation. Typically, expansion of both stents can be done one right after the other after proper placement of the first and second balloons.

## Claims

### 1. A bifurcated stent (200) comprising:

a proximal tubular section (210);  
a first distal tubular section (220), said first distal tubular section (220) connected to said proximal section (210) by connector members (250); and  
a second distal tubular section (230), said first (220) and second (230) distal tubular sections welded together (260) at their proximal end (225,235), **characterised in that,**  
the weld is a spot weld formed between a dowel (261) and a hole (262),

the connector members (250) are omega-shaped; and  
the connector members (250) are continuously placed (240) around the circumference of the first distal section (220).

2. A The stent of claim 1 wherein the shape of the connector members (250) is different than the struts (211, 211) shape of forming the proximal (210) and distal (220, 230) sections.
3. The stent of claim 1 wherein said distal (220, 230) and said proximal (210) sections are expandable to different diameters.

## Patentansprüche

### 1. Gabelförmiger Stent (200), der folgendes aufweist:

einen proximalen röhrenförmigen Abschnitt (210);  
einen ersten distalen röhrenförmigen Abschnitt (220), wobei der erste distale röhrenförmige Abschnitt (220) mit dem proximalen Abschnitt (210) durch Verbindungselemente (250) verbunden ist; und  
einen zweiten distalen röhrenförmigen Abschnitt (230), wobei der erste (220) und der zweite (230) distalen röhrenförmigen Abschnitt an ihren proximalen Enden (225, 235) miteinander verschweißt sind (260), **dadurch gekennzeichnet, daß** die Verschweißung eine Punktverschweißung ist, die zwischen einem Dübel (261) und einem Loch (262) gebildet ist, die Verbindungselemente (250) omega-förmig sind; und die Verbindungselemente (250) kontinuierlich um den Umfang des ersten distalen Abschnitts (220) angeordnet sind (240).

2. Stent nach Anspruch 1, wobei die Form der Verbindungselemente (250) unterschiedlich ist zu der Form der Streben (211, 211), welche den proximalen Abschnitt (210) und die distalen Abschnitte (220, 230) bilden.
3. Stent nach Anspruch 1, wobei die distalen Abschnitte (220, 230) und der proximale Abschnitt (210) auf unterschiedliche Durchmesser expandierbar sind.

## Revendications

### 1. Stent bifurqué (200) comprenant :

une section tubulaire proximale (210) ;  
une première section tubulaire distale (220), ladite première section tubulaire distale (220)

étant raccordée à ladite section proximale (210)  
par des éléments de connecteur (250) ; et  
une seconde section tubulaire distale (230), les-  
dites première (220) et seconde (230) sections  
tubulaires distales étant soudées ensemble 5  
(260) au niveau de leurs extrémités proximales  
(225, 235), **caractérisé en ce que:**

la soudure est une soudure par points for-  
mée entre une goupille de positionnement 10  
(261) et un trou (262), les éléments de con-  
necteur (250) sont en forme d'omega ; et  
les éléments de connecteur (250) sont pla-  
cés de manière continue (240) autour de la  
circonférence de la première section distale 15  
(220).

2. Stent selon la revendication 1, dans lequel la forme  
des éléments de connecteur (250) est différente de 20  
la forme des entretoises (211, 211) formant les sec-  
tions proximale (210) et distales (220, 230).
3. Stent selon la revendication 1, dans lequel lesdites  
sections distale (220, 230) et proximale (210) sont 25  
extensibles jusqu'à différents diamètres.

30

35





40

45


50

55




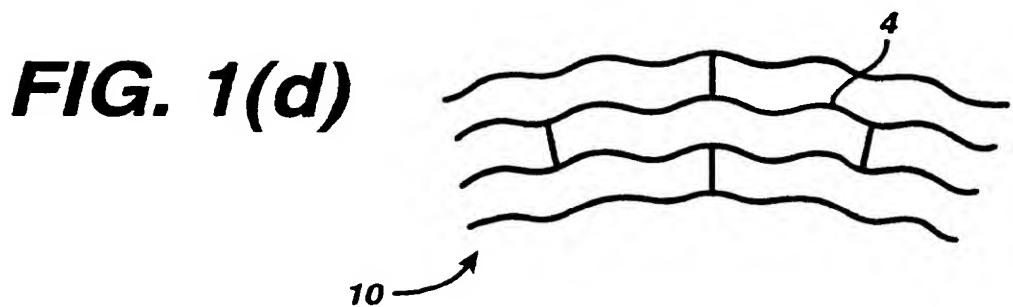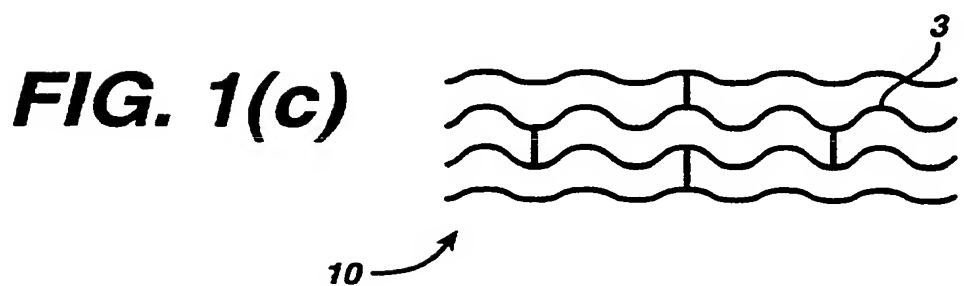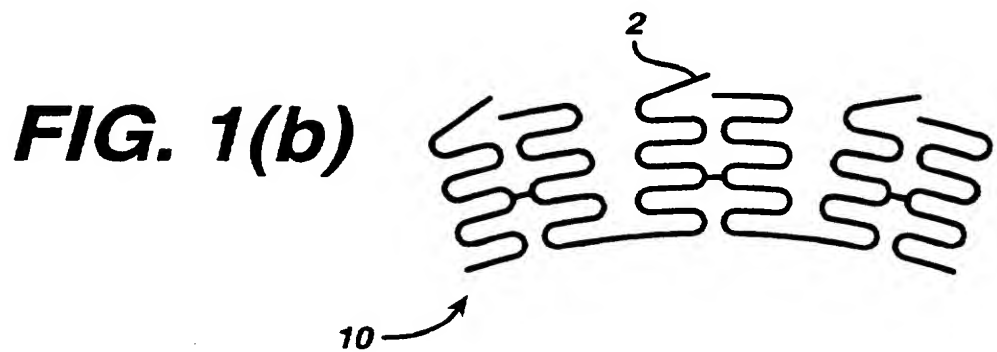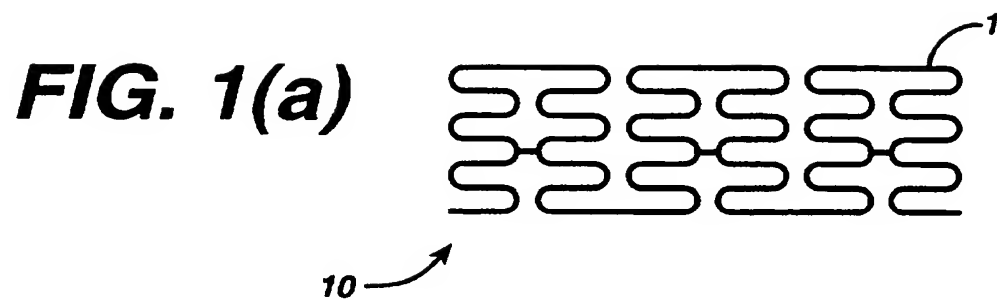


**FIG. 2**

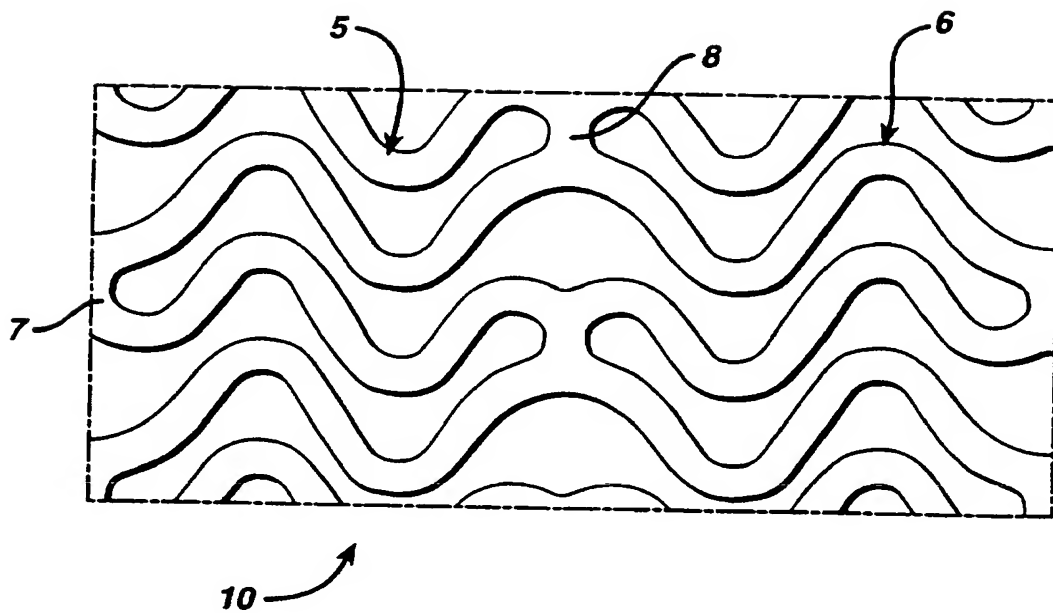


**FIG. 3(a)**

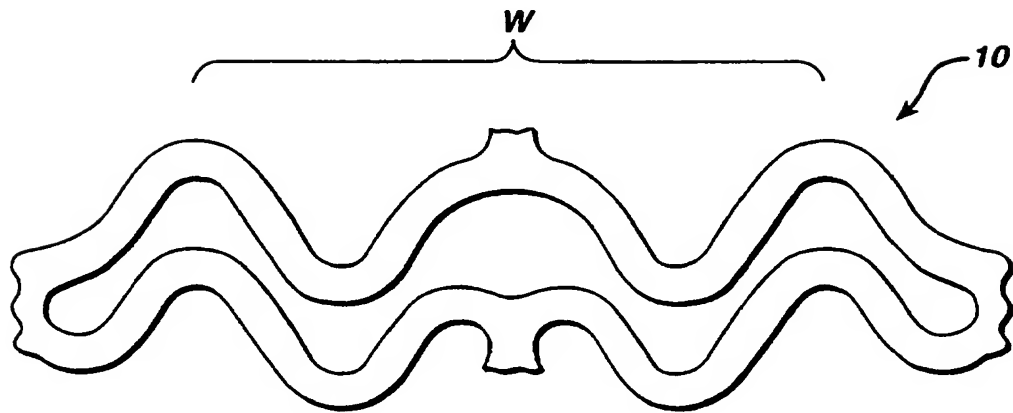

**FIG. 3(b)**

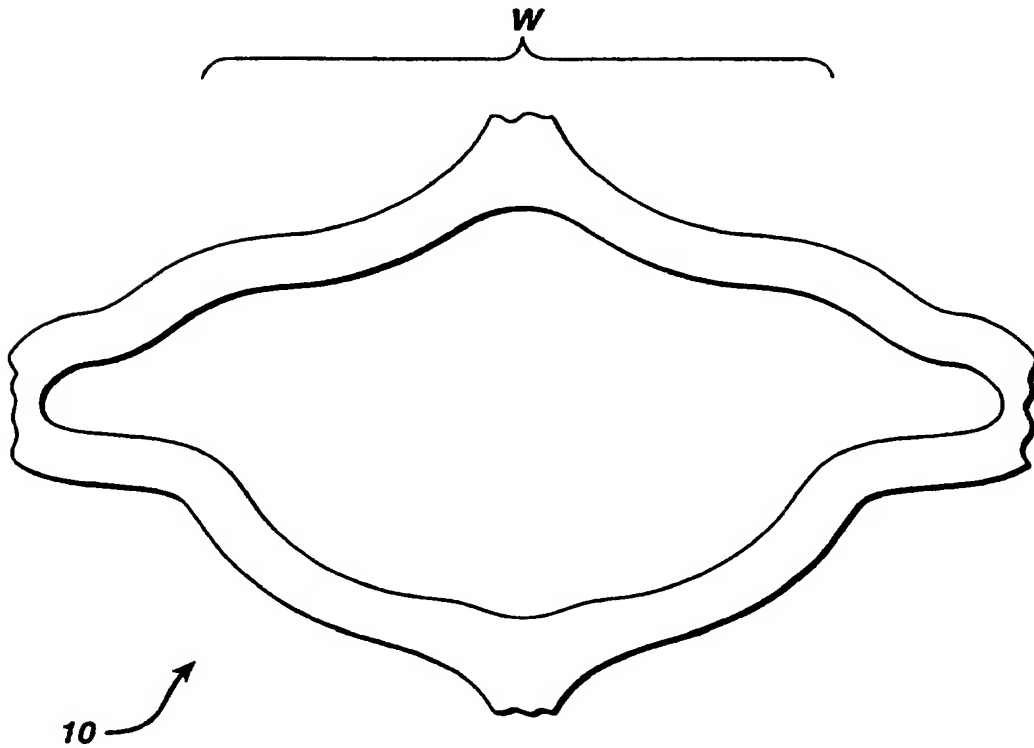

**FIG. 4**

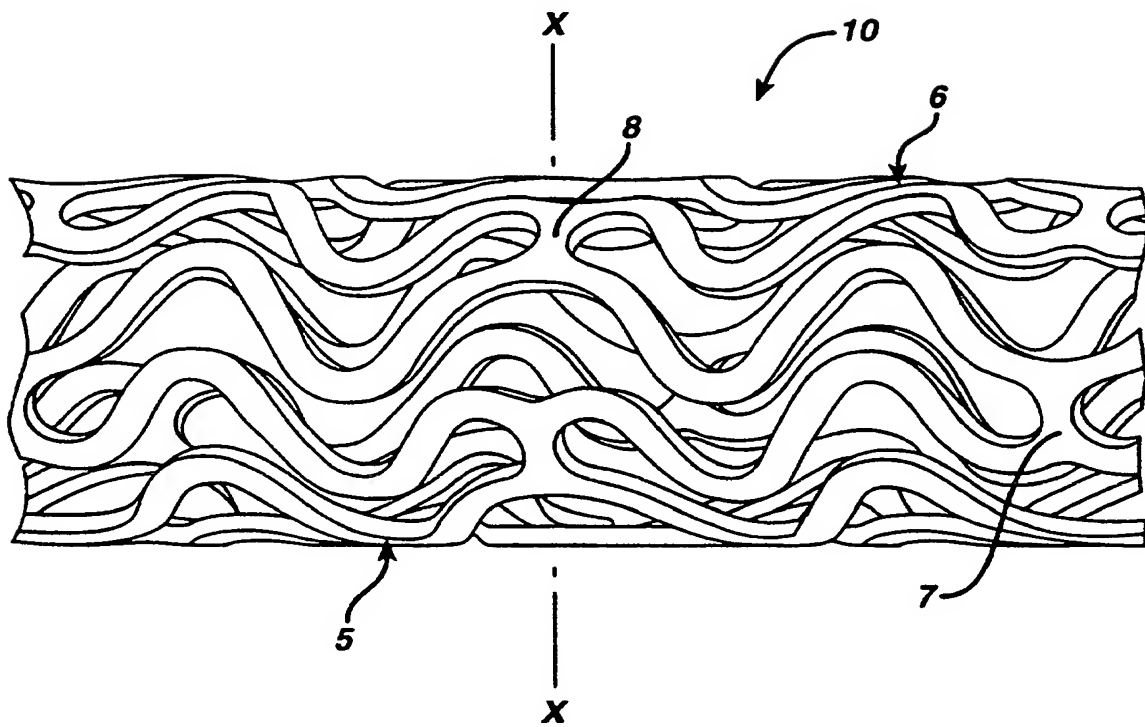

**FIG. 5**



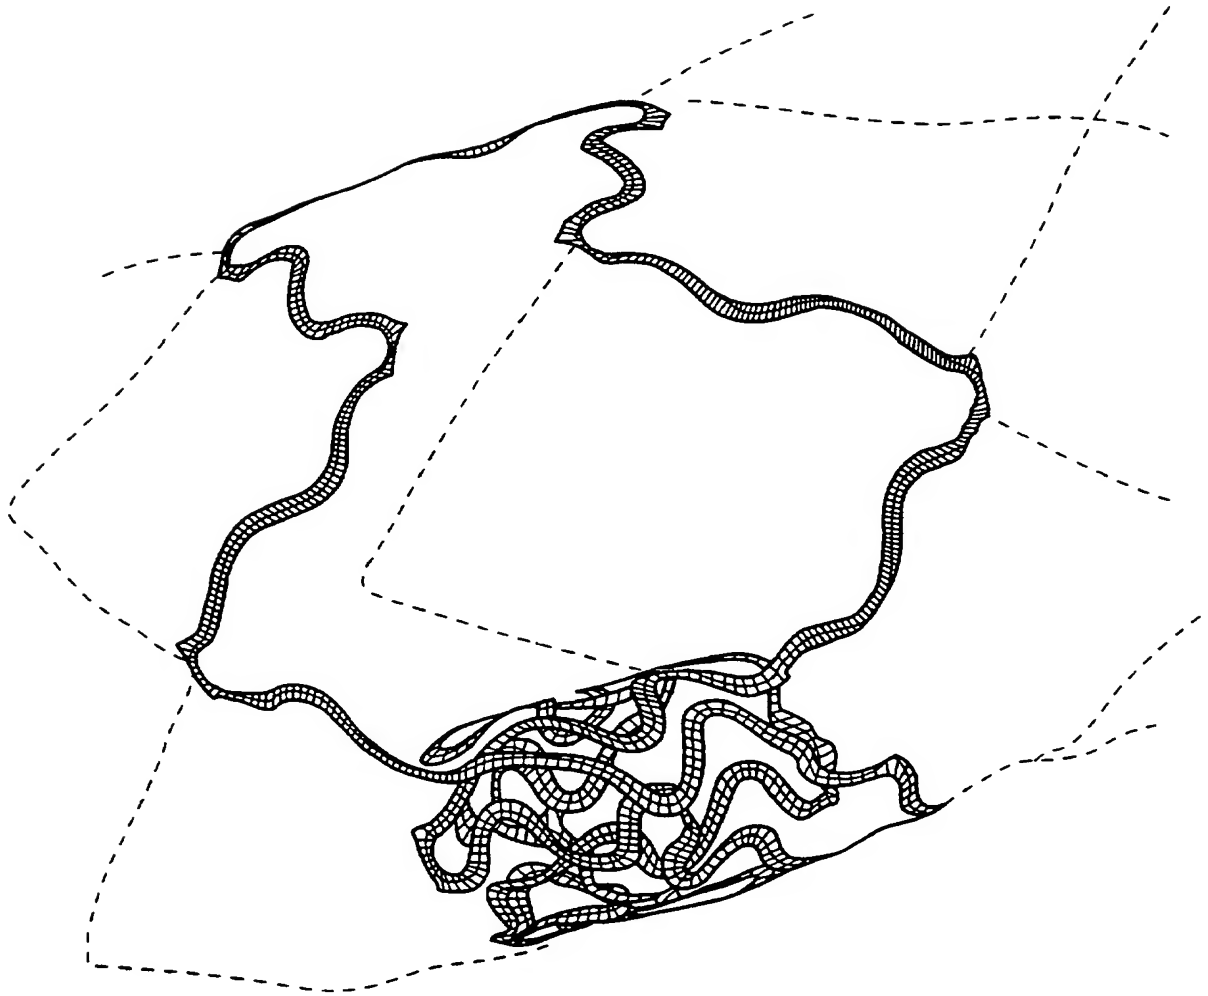



FIG. 6

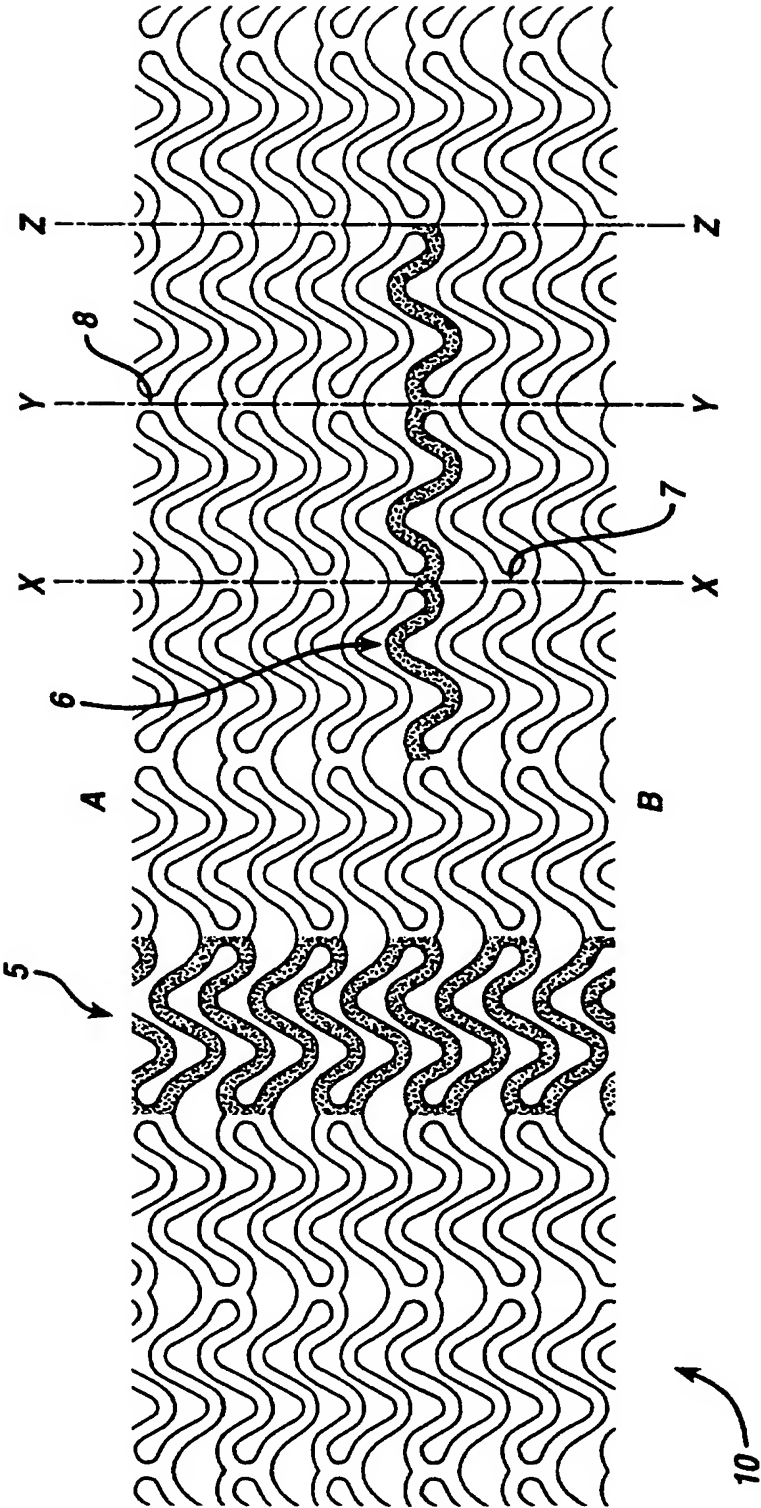

**FIG. 7**

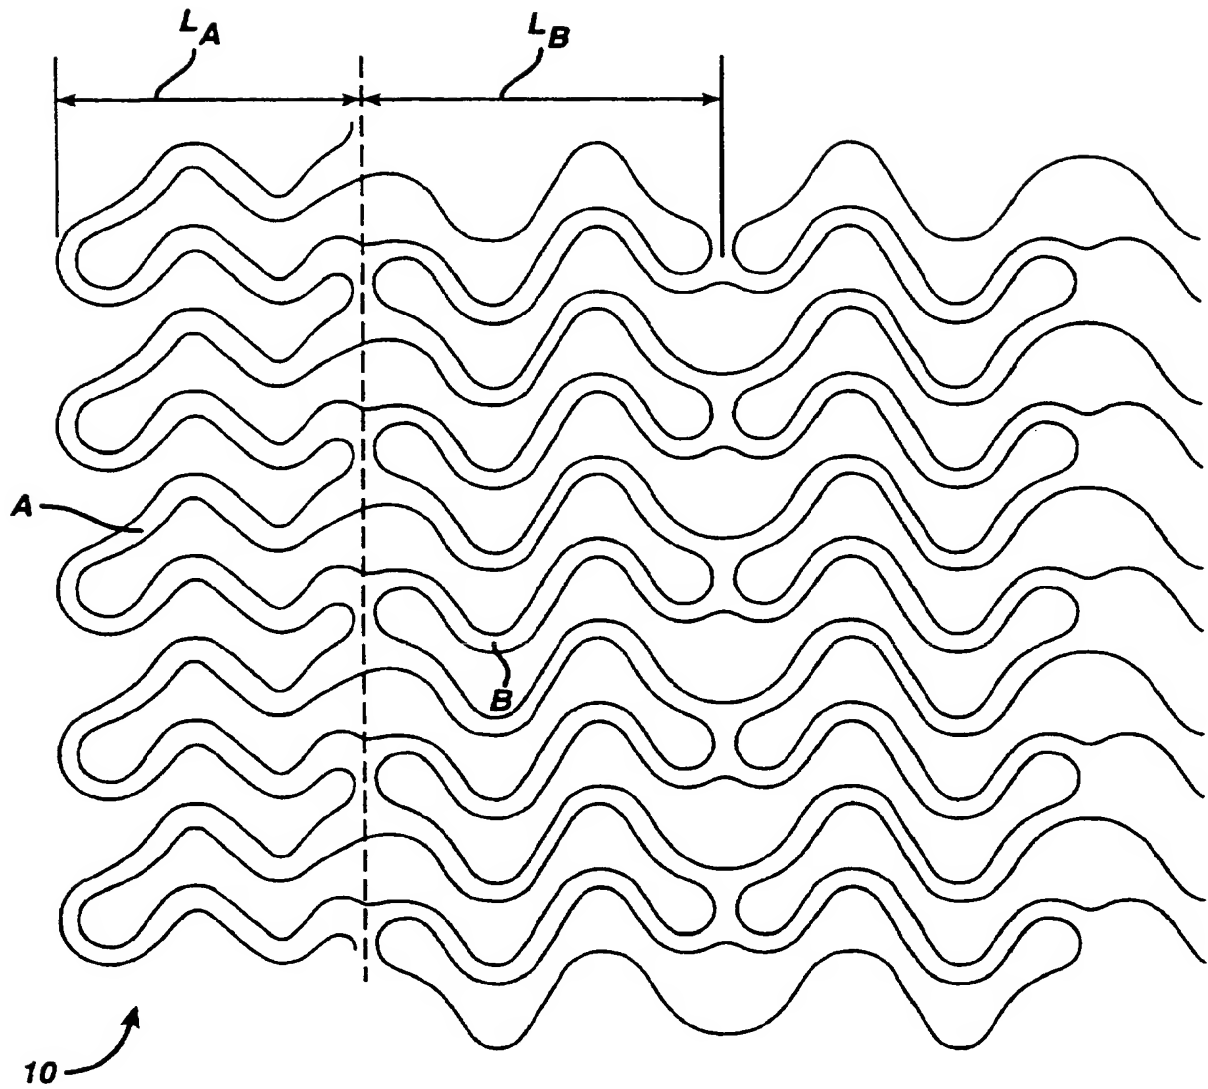


**FIG. 8**

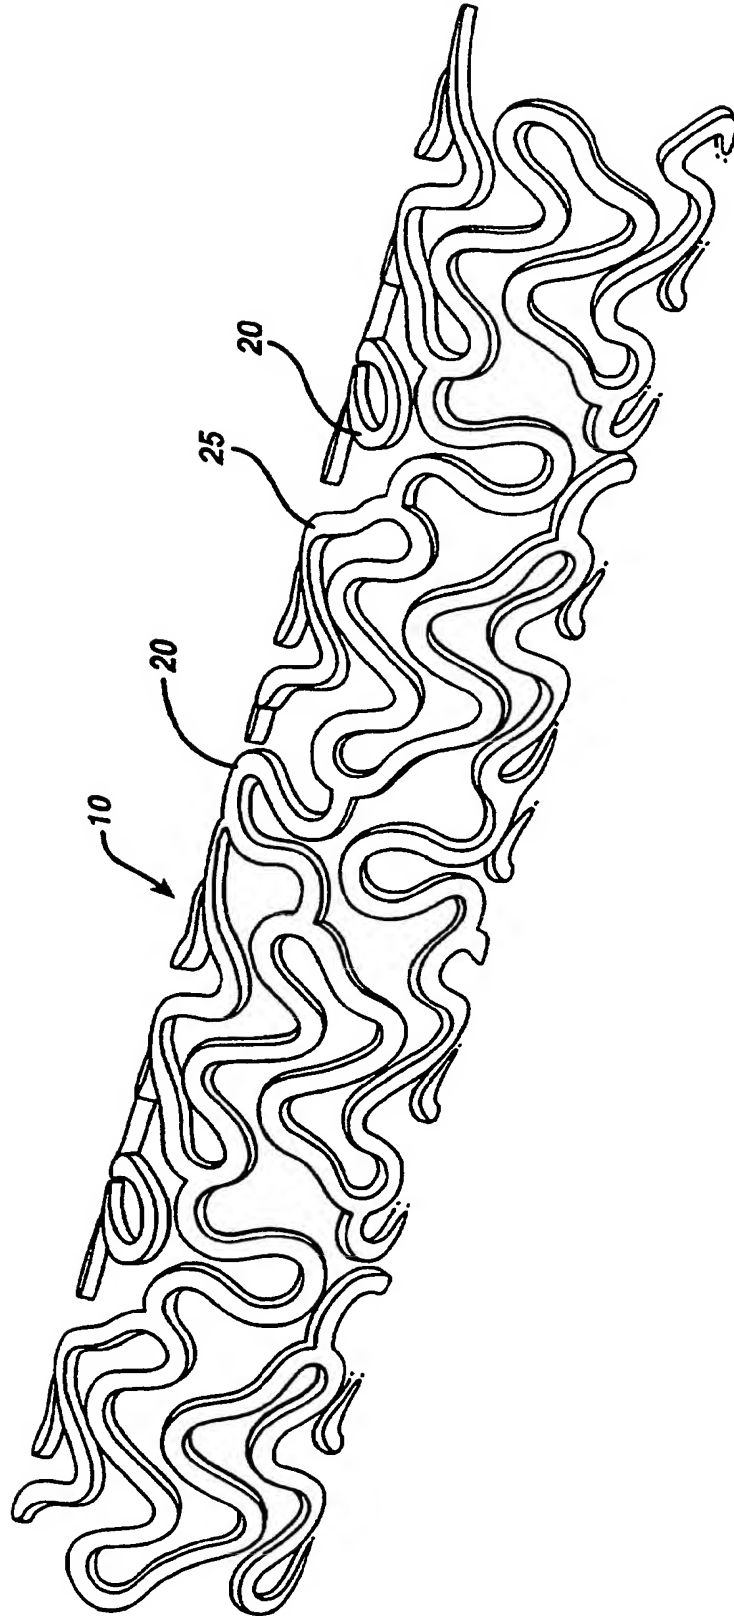





**FIG. 9**

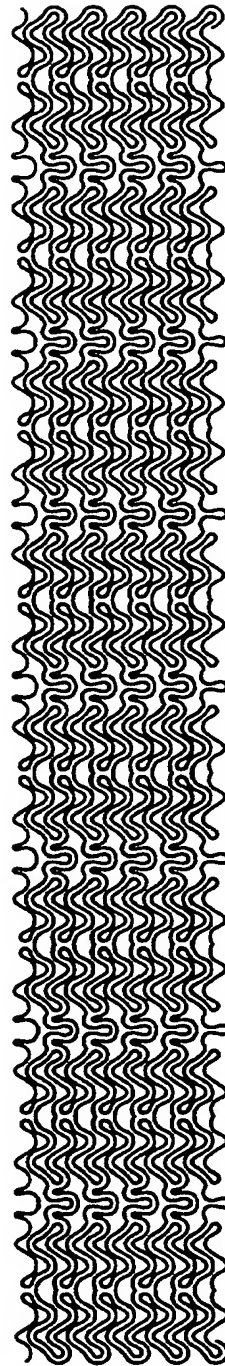


**FIG. 10**

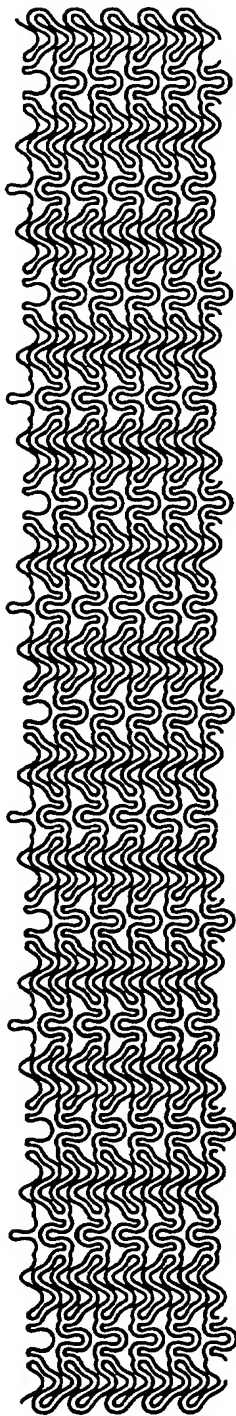


**FIG. 11**

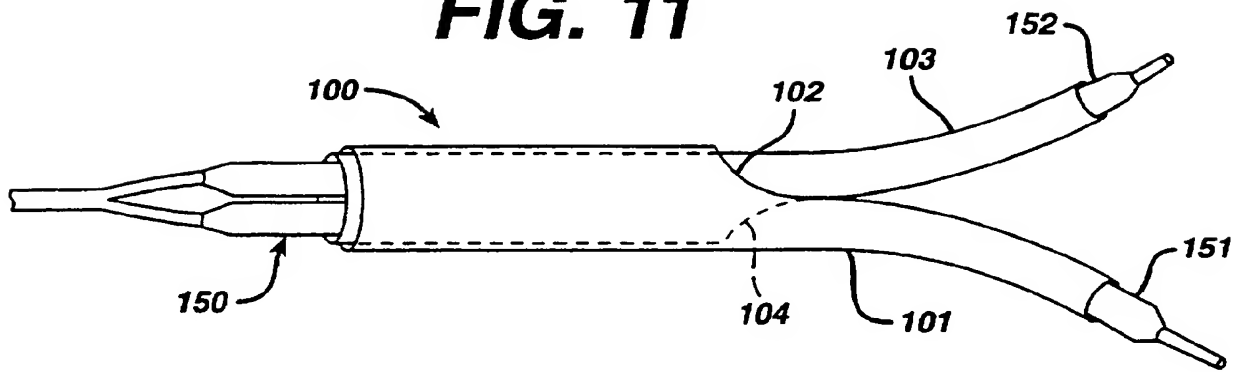


**FIG. 12**

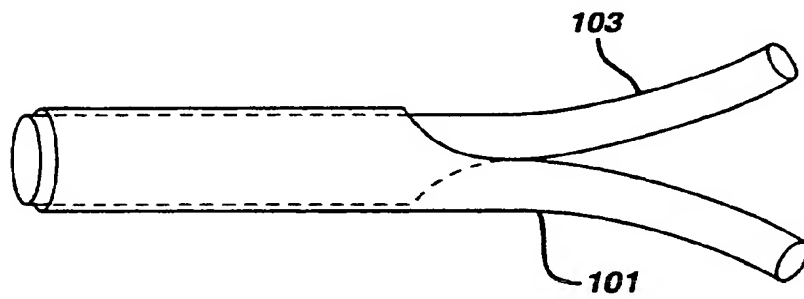

**FIG. 13**

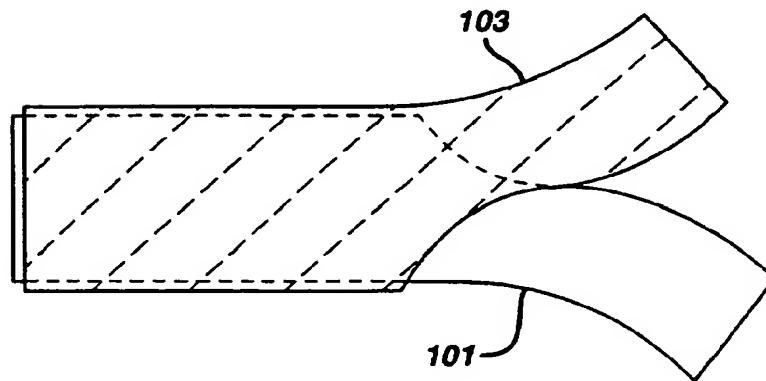

**FIG. 14**

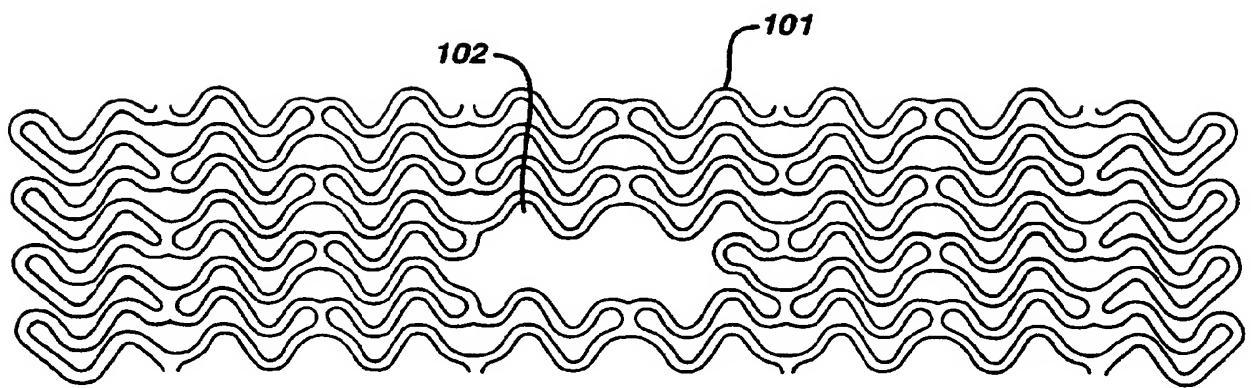

**FIG. 15**

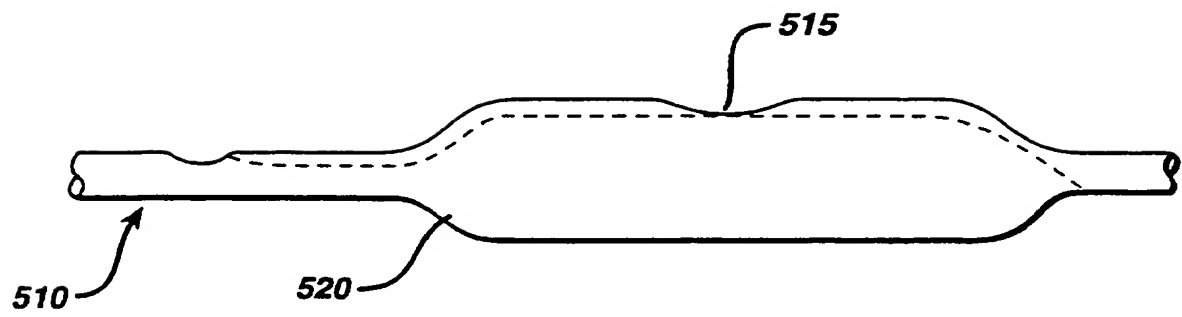


FIG. 16




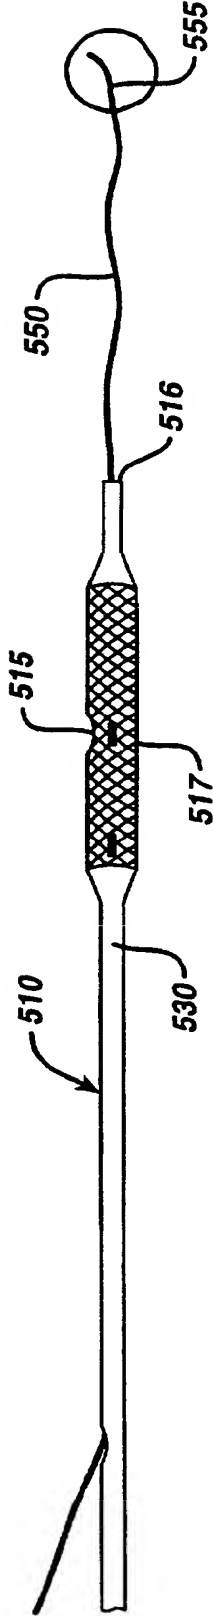


FIG. 17

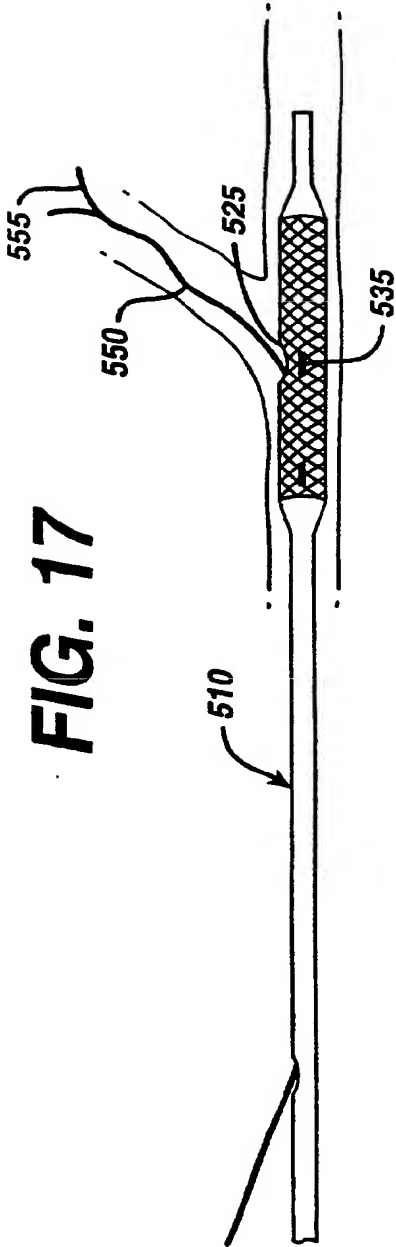

**FIG. 18**

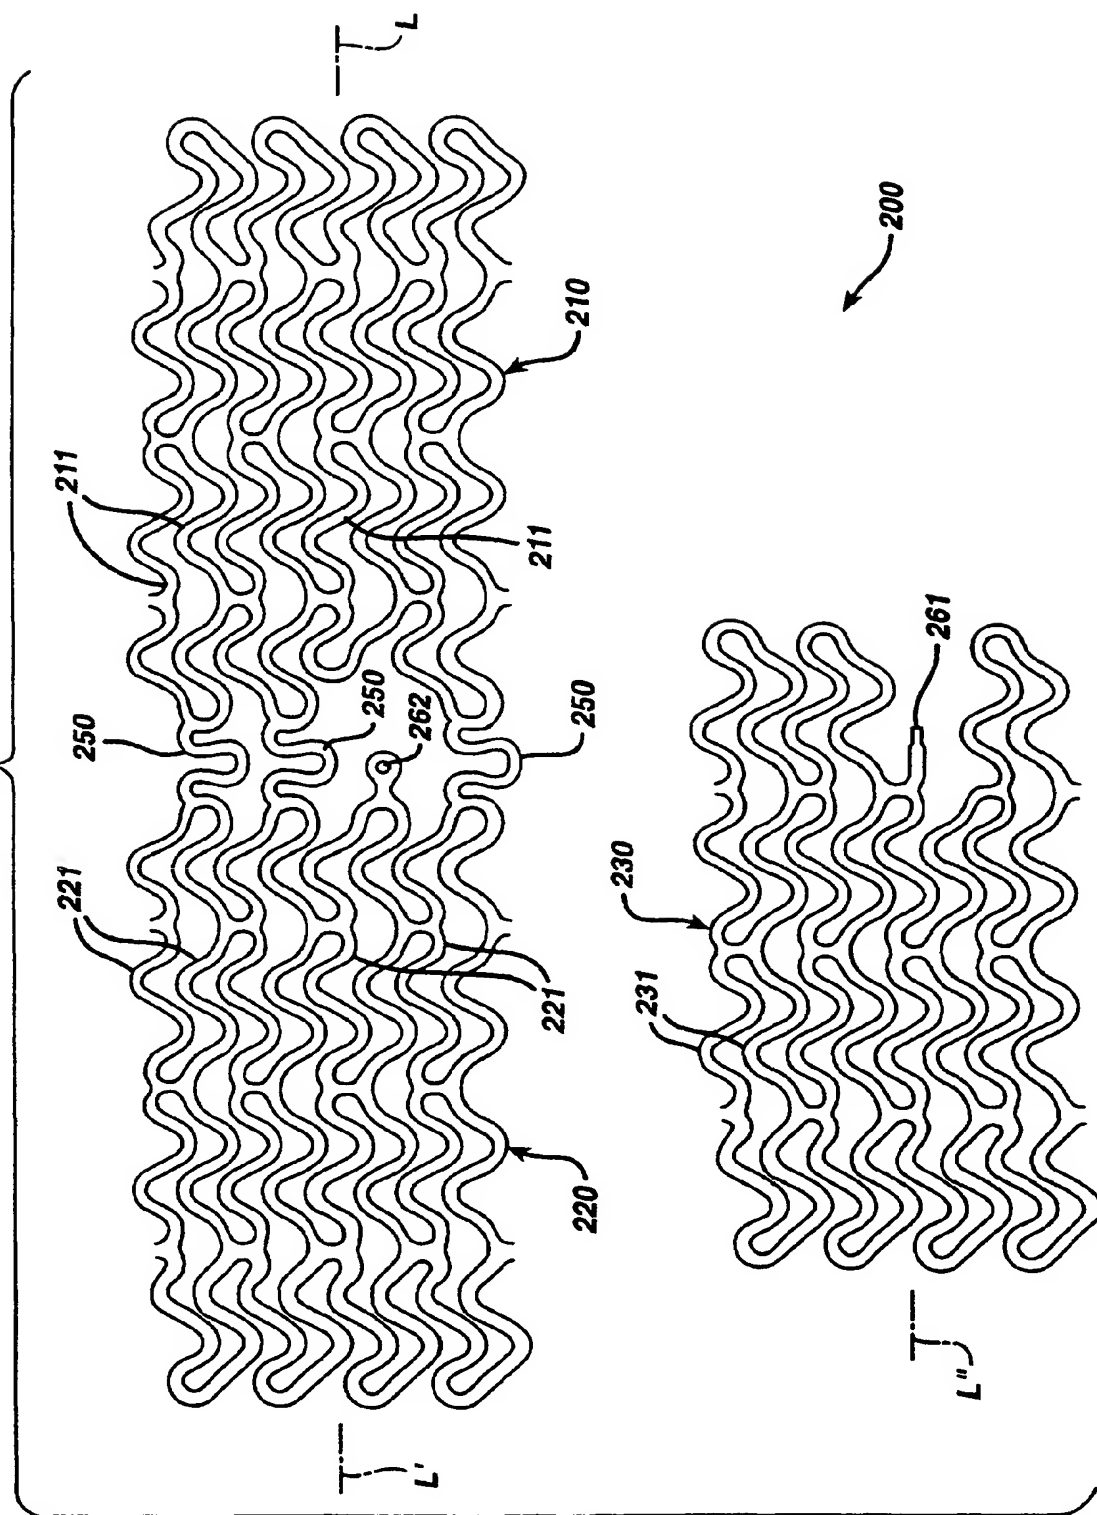

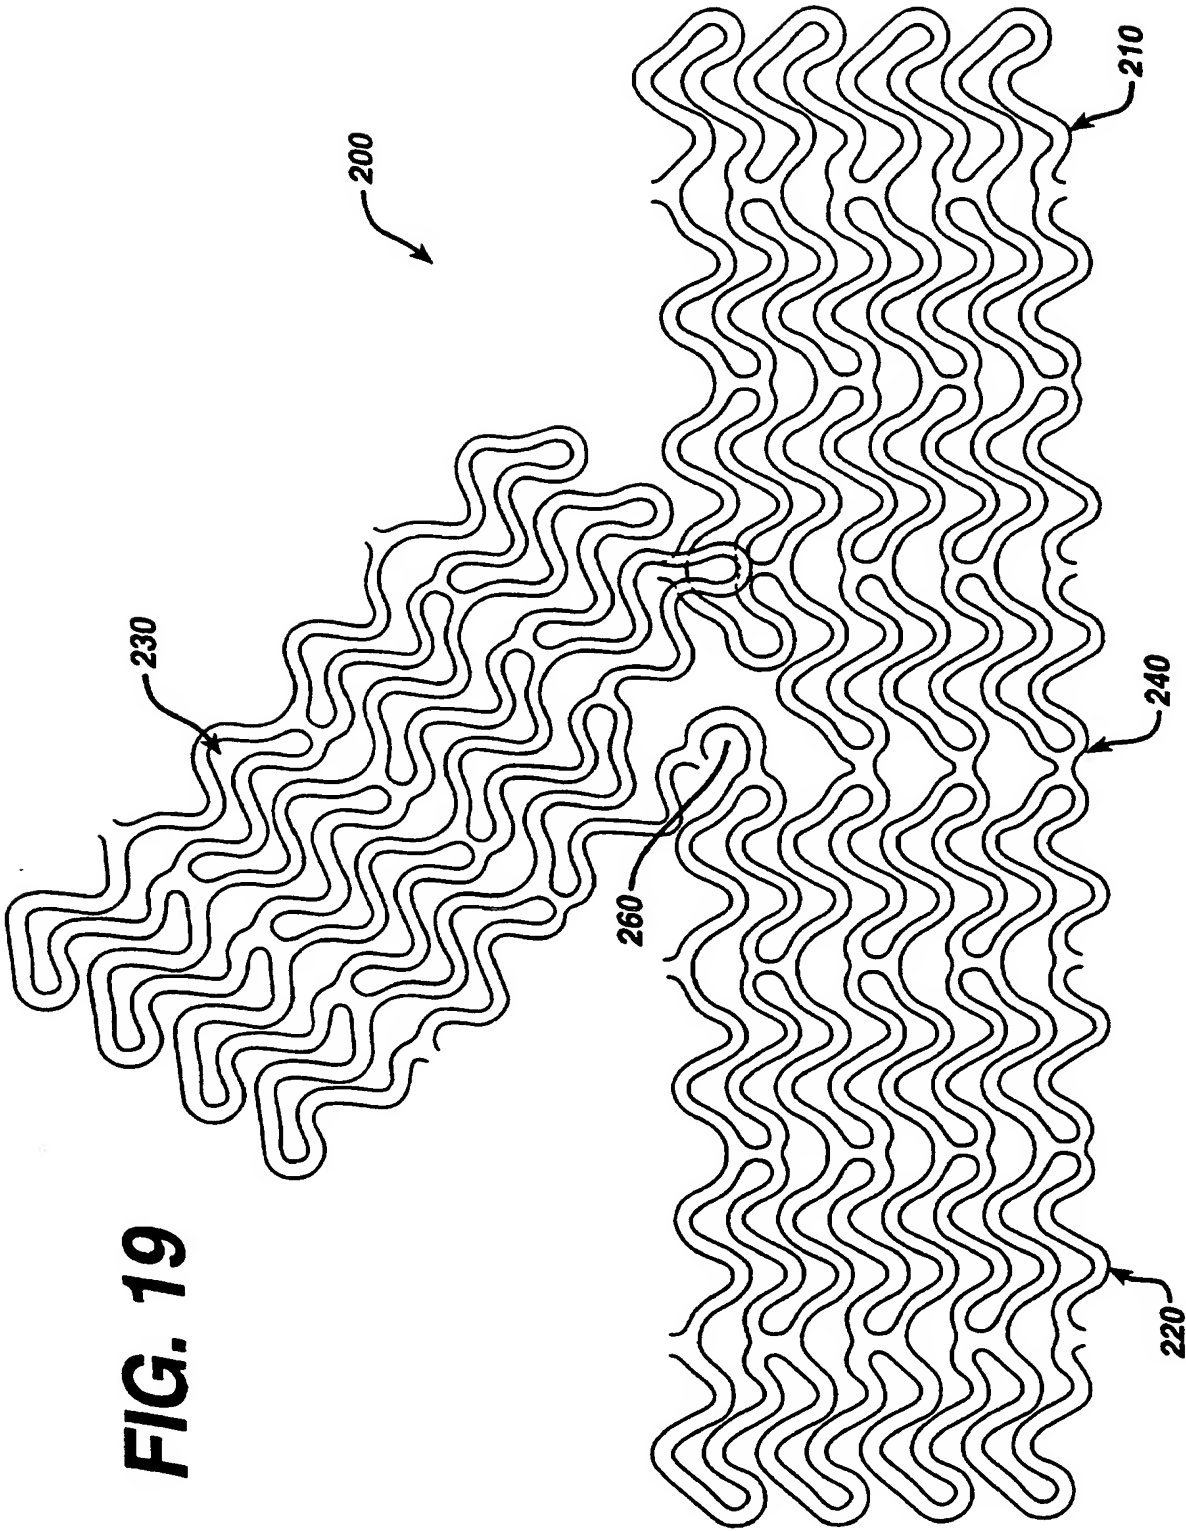



**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- FR 2733682 [0011]
- US 5108415 A [0059]
- US 5156612 A [0059]
- US 5304197 A [0059]